

APPLICATION NOTE



Subject : Analysis of 10 kinds of amino acid among the amino acid material

▶ **Analysis condition**


Mobile phase : A(Na328)/B(Na740) Binary Gradient

Flow rate : 0.3 ml/min

Detection wavelength : 570nm

Sample injection : 20uL

▶ **Chromatogram**

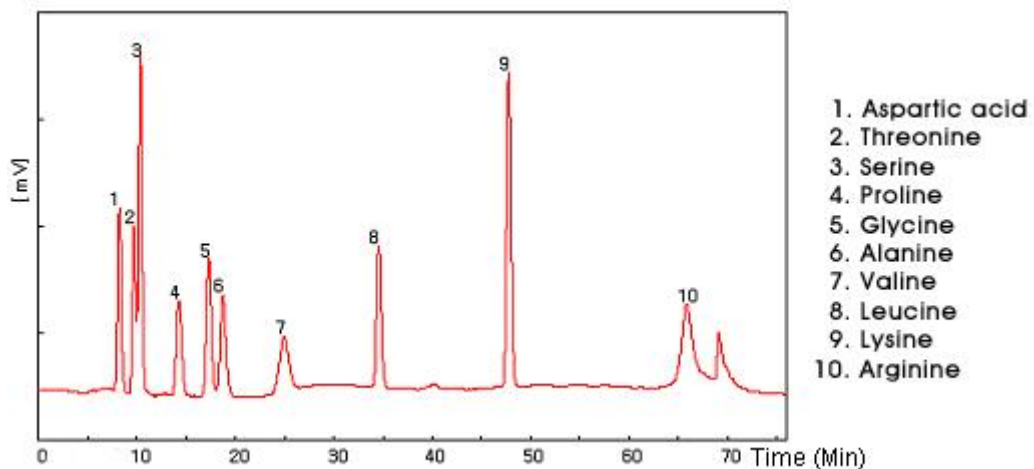

영린기기

431-836 경기도 안양시 동안구 호계2동 899-6 Tel : 031-428-8700 Fax : 031-428-8787
Homepage : www.younglin.com E-mail : sales@younglin.com