



APPLICATION NOTE

**Subject : Analysis of 13 kinds of amino acid
among the amino acid material**

▶ Analysis condition


Mobile phase : A(Na328)/B(Na740) Binary Gradient

Flow rate : 0.3ml/min

Detection wavelength : 570 nm

Sample injection : 20uL

▶ Chromatogram

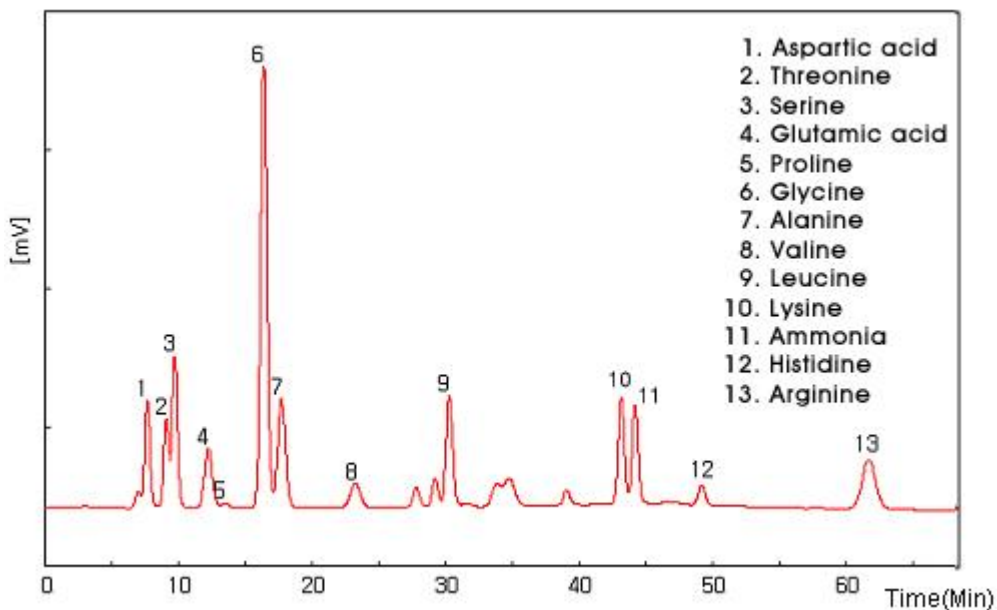

영린기기

431-836 경기도 안양시 동안구 호계2동 899-6 Tel : 031-428-8700 Fax : 031-428-8787
Homepage : www.younglin.com E-mail : sales@younglin.com